



VanishPoint Syringes


Standard Draw Procedure

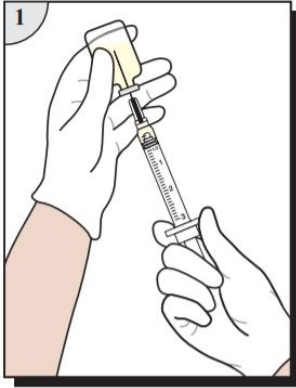

In-Patient, Automated Retraction

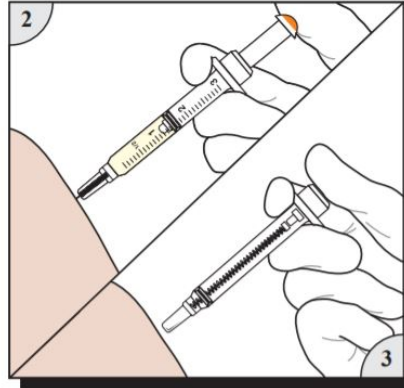

Non-Reusable

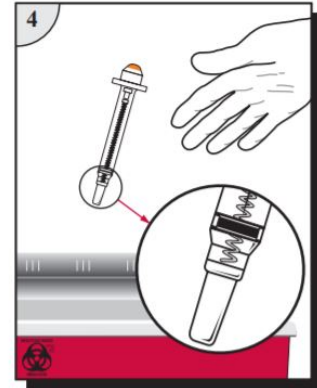

- For injection into patients, continue depressing plunger to activate automatic needle retraction while needle is still in patient.
- Needle will automatically retract into syringe, preventing exposure to contaminated needle and rendering syringe non-reusable. In the event that needle retraction mechanism does not activate, discard syringe in an appropriate sharps container per protocol of institution. Do not recap contaminated needles.